


3-chloro-1-butene in CDCl₃



NAME Jun19-2015
EXPNO 1
PROCNO 1
Date 20150619
Time 10.43
INSTRUM spect
PROBHD 5 mm QNP 1H/13
PULPROG zg30
TD 32768
SOLVENT CDCl₃
NS 16
DS 2
SWH 4901.961 Hz
FIDRES 0.149596 Hz
AQ 3.3423860 sec
RG 128
DW 102.000 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 11.50 usec
PL1 0.00 dB
SFO1 300.2598500 MHz
SI 16384
SF 300.2580132 MHz
WDW EM
SSB 0
LB 0.25 Hz
GB 0
PC 1.00

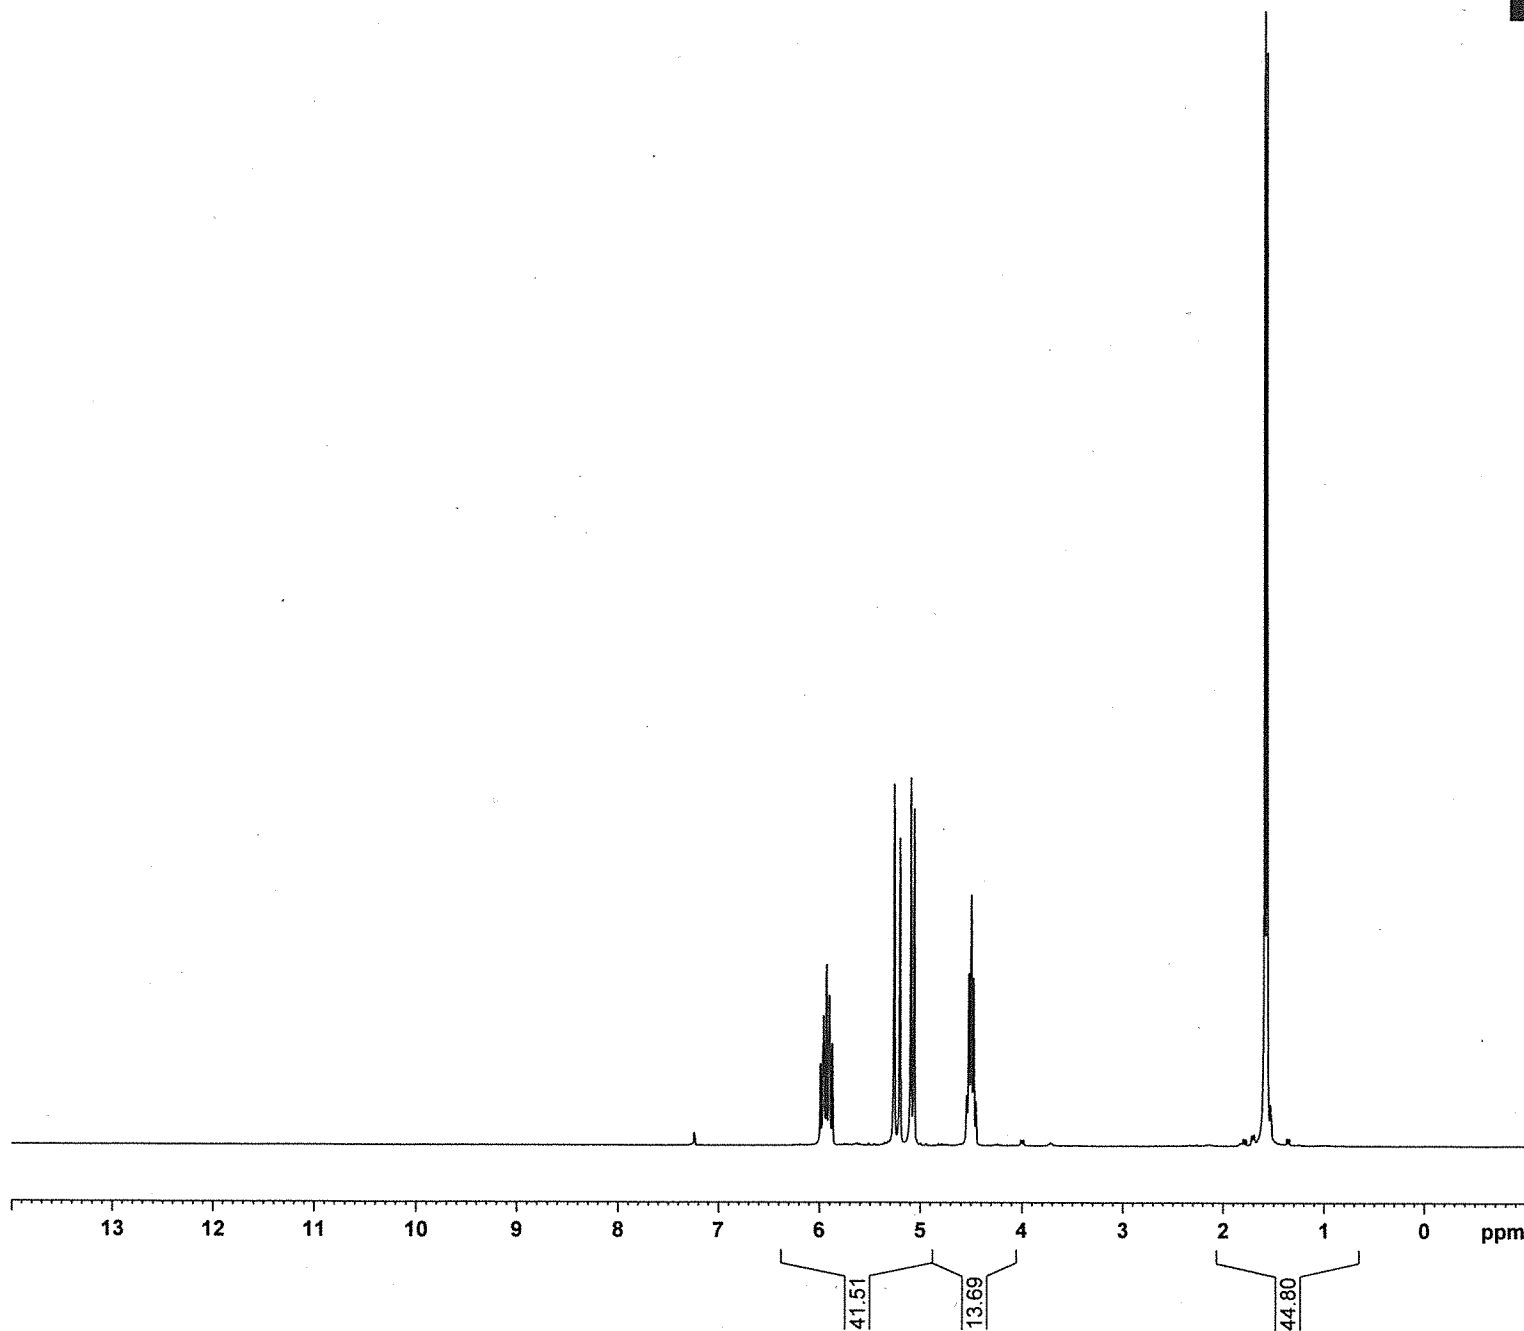

Acquisition Time (sec)	3.3423	Comment	3-chloro-1-butene in CDCl ₃	Date	19 Jun 2015 10:44:32
Date Stamp	19 Jun 2015 10:44:32				
File Name	\\netdrive.uvic.ca\SFGClients\Science\Chemistry\UGNMR\data\ugnmruser\nmr\Jun19-2015\1\data\1\1r			Frequency (MHz)	300.26
Nucleus	¹ H	Number of Transients	16	Origin	spect
Owner	ugnmruser	Points Count	16384	Original Points Count	16384
SW(cyclical) (Hz)	4901.96	Pulse Sequence	zg30	Receiver Gain	128.00
Spectrum Type	STANDARD	Solvent	CHLOROFORM-d	Spectrum Offset (Hz)	1836.7882
		Sweep Width (Hz)	4901.66	Temperature (degree C)	27.000

