


2,6-diisopropylaniline in CDCl₃



NAME May14-2014
 EXPNO 3
 PROCNO 1
 Date_ 20140514
 Time 10.58
 INSTRUM spect
 PROBHD 5 mm QNP 1H/13
 PULPROG zg30
 TD 32768
 SOLVENT CDCl₃
 NS 16
 DS 2
 SWH 4901.961 Hz
 FIDRES 0.149596 Hz
 AQ 3.3423860 sec
 RG 32
 DW 102.000 usec
 DE 6.50 usec
 TE 673.2 K
 D1 1.00000000 sec
 TDO 1

===== CHANNEL f1 =====
 NUC1 1H
 P1 11.50 usec
 PL1 0.00 dB
 SFO1 300.2598500 MHz
 SI 16384
 SF 300.2580132 MHz
 WDW EM
 SSB 0
 LB 0.25 Hz
 GB 0
 PC 1.00

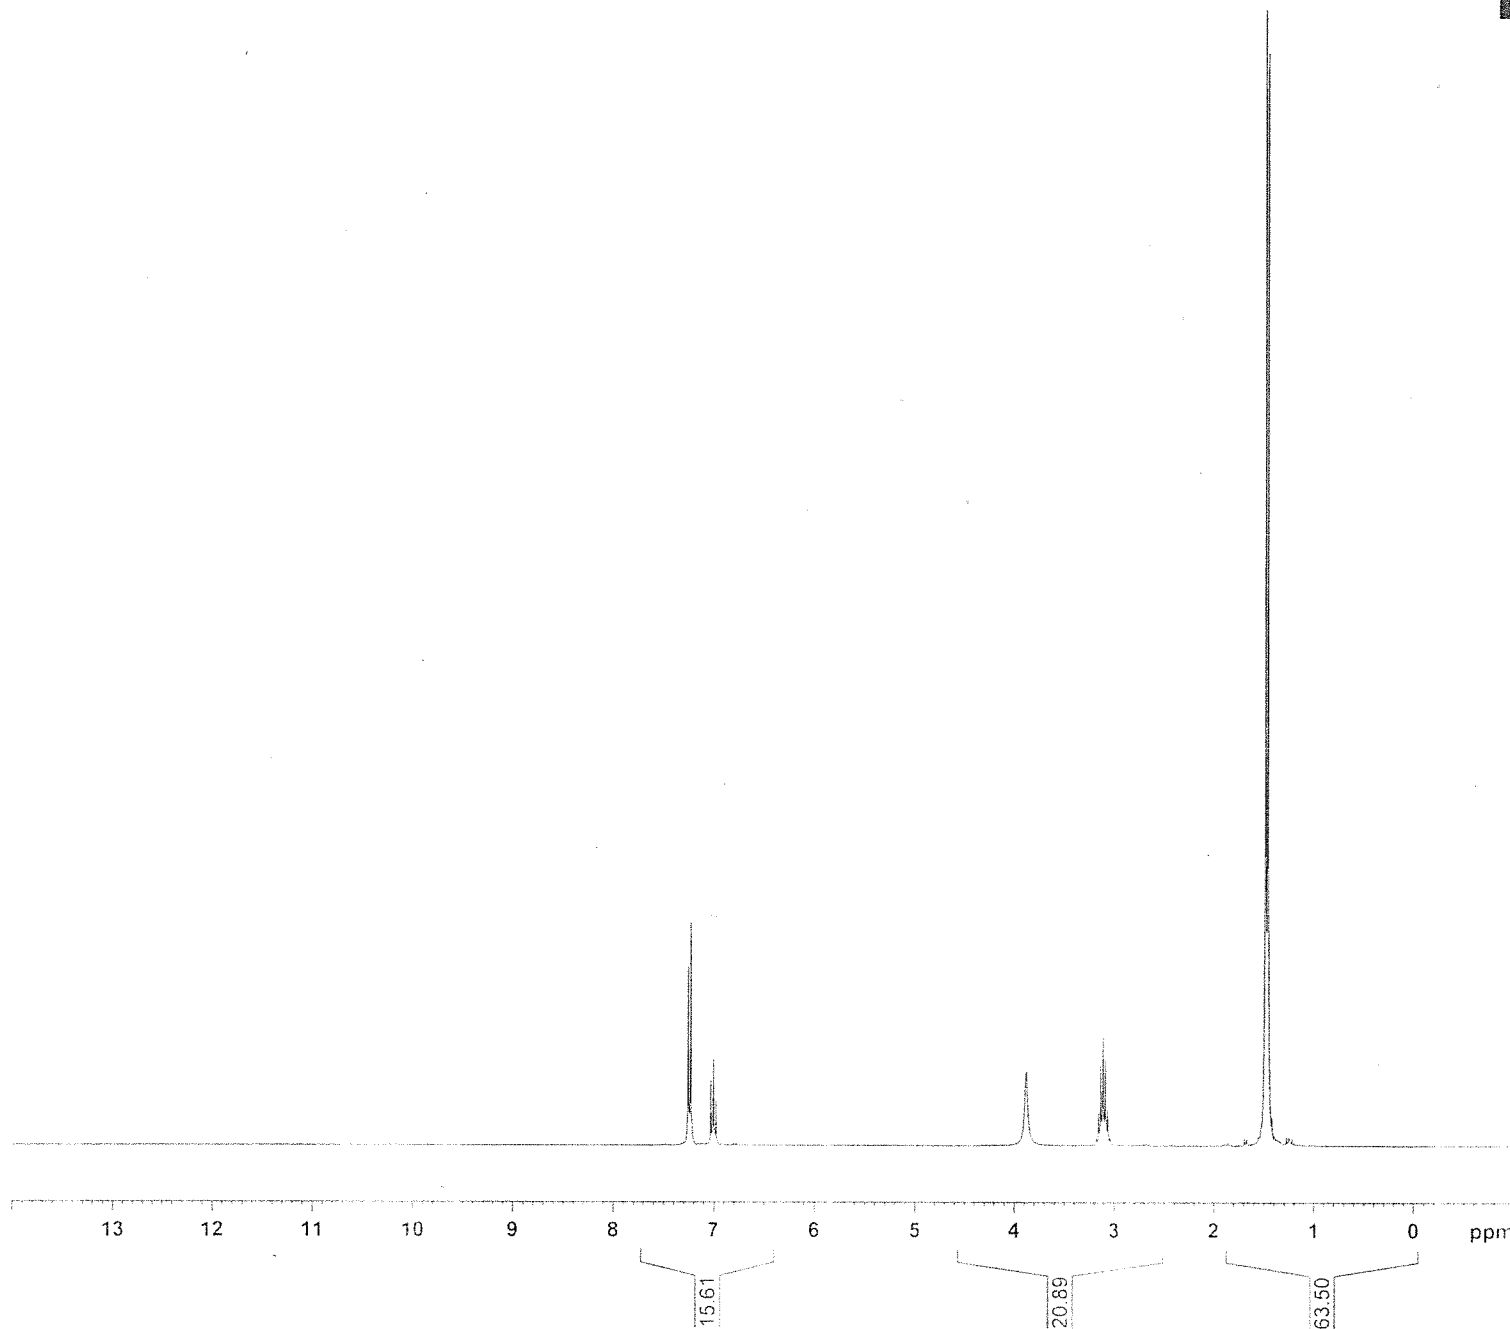

Acquisition Time (sec)	3.3423	Comment	2,6-diisopropylaniline in CDCl ₃	Date	14 May 2014 10:57:20
Date Stamp	14 May 2014 10:57:20				
File Name	\\netdrive.uvic.ca\\SFGC\\lients\\Science\\Chemistry\\UGNMR\\data\\ugnmruser\\nmr\\May14-2014\\3\\pdata\\1\\1r			Frequency (MHz)	300.26
Nucleus	¹ H	Number of Transients	16	Origin	spect
Owner	ugnmruser	Points Count	16384	Pulse Sequence	zg30
SW(cyclical) (Hz)	4901.96	Solvent	CHLOROFORM-d	Receiver Gain	32.00
Spectrum Type	STANDARD	Sweep Width (Hz)	4901.66	Spectrum Offset (Hz)	1836.7882

