

3,4-dibromothiophene in CDCl₃


132.23
124.69
124.61
124.12
123.63
114.27
113.73
113.37
77.85
77.43
77.00
64.28
64.14
63.97



NAME May25-2015
EXPNO 14
PROCNO 1
Date 20150525
Time 15.10
INSTRUM spect
PROBHD 5 mm QNP 1H/13
PULPROG zgpg30
TD 32768
SOLVENT CDCl₃
NS 400
DS 4
SWH 18248.176 Hz
FIDRES 0.556890 Hz
AQ 0.8978932 sec
RG 23170.5
DW 27.400 usec
DE 6.50 usec
TE 299.8 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 13C
P1 17.70 usec
PL1 -2.00 dB
SFO1 75.5082390 MHz

===== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 80.00 usec
PL2 0.00 dB
PL12 16.85 dB
PL13 60.00 dB
SFO2 300.2593512 MHz
SI 16384
SF 75.4999178 MHz
WDW EM
SSB 0
LB 1.20 Hz
GB 0
PC 1.40

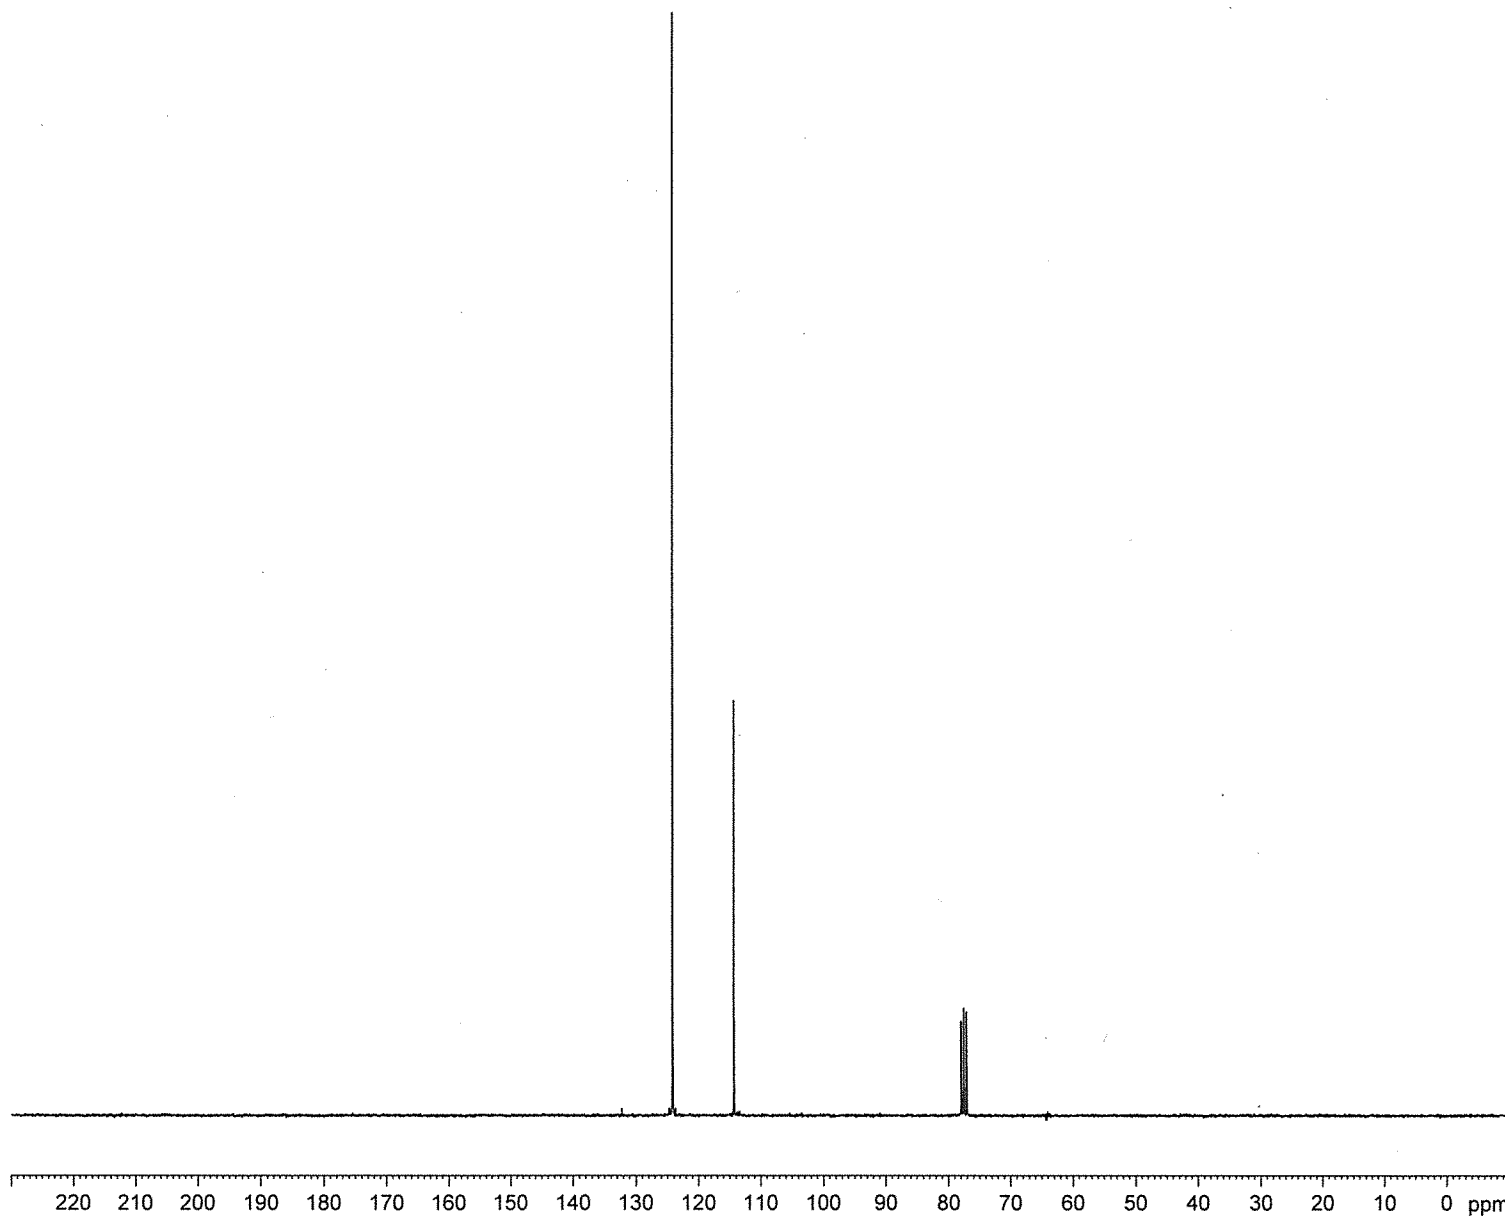

Acquisition Time (sec)	0.8978	Comment	3,4-dibromothiophene in CDCl3			Date	25 May 2015 15:11:12	
Date Stamp	25 May 2015 15:11:12							
File Name	\\netdrive.uvic.ca\\SFGClients\\Science\\Chemistry\\UGNMR\\data\\ugnmruser\\nmr\\May25-2015\\14\\pdata\\1\\1r					Frequency (MHz)	75.50	
Nucleus	13C	Number of Transients	400	Origin	spect	Original Points Count	16384	
Owner	ugnmruser	Points Count	16384	Pulse Sequence	zgpg30	Receiver Gain	23170.50	
SW(cyclical) (Hz)	18248.18	Solvent	CHLOROFORM-d	Spectrum Offset (Hz)	8321.2246	Spectrum Type	STANDARD	
Sweep Width (Hz)	18247.06	Temperature (degree C)	26.800					

